


Separation of Dithianone

Data# B-046

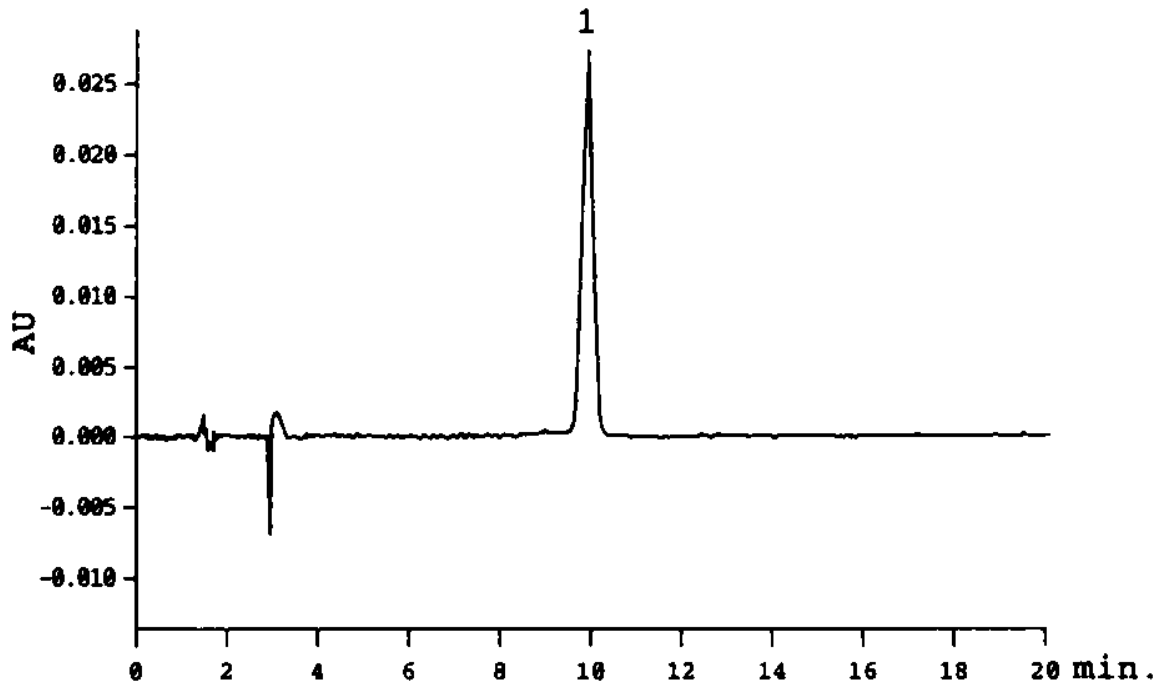

Column	Mightysil RP-18 GP 150-4.6mmØ 5µm
Eluent	Water / Methanol / Acetic acid = 40 / 60 / 1
Flow Rate	1.0mL / min.
Detection	UV330nm
Temperature	40
Sample Volume	10µl
Detected peaks	1. Dithianone 50 mg / ml