


## Separation of Peptides

Data# B-075

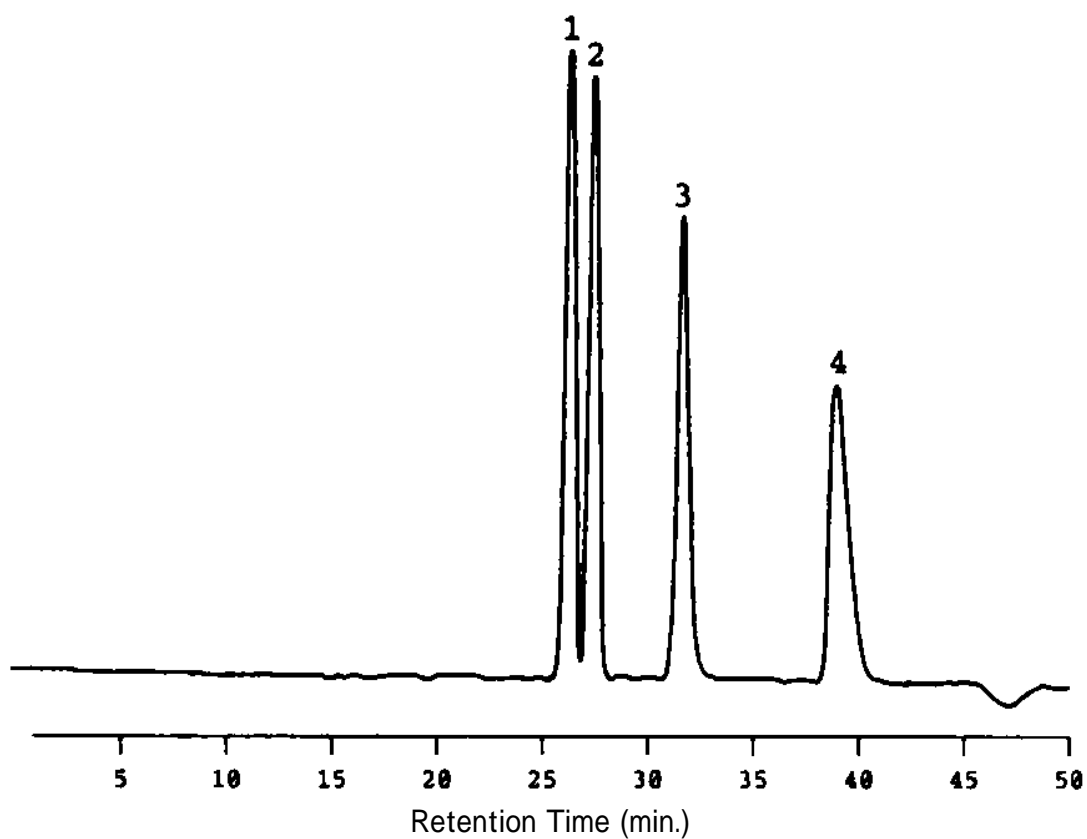

Column	Mightysil RP-18 GP Aqua 250-4.6mmØ 5µm	
Eluent	100% Water	
Flow Rate	0.1mL / min.	
Detection	RI	
Temperature	35	
Sample Volume	5µl	
Detected peaks	1. Alanine(Ala)	0.2 mg / mL
	2. Ala-Ala	0.2 mg / mL
	3. Ala-Ala-Ala	0.2 mg / mL
	4. Ala-Ala-Ala-Ala	0.2 mg / mL