


Separation of Preservatives - 1

Data# F-043

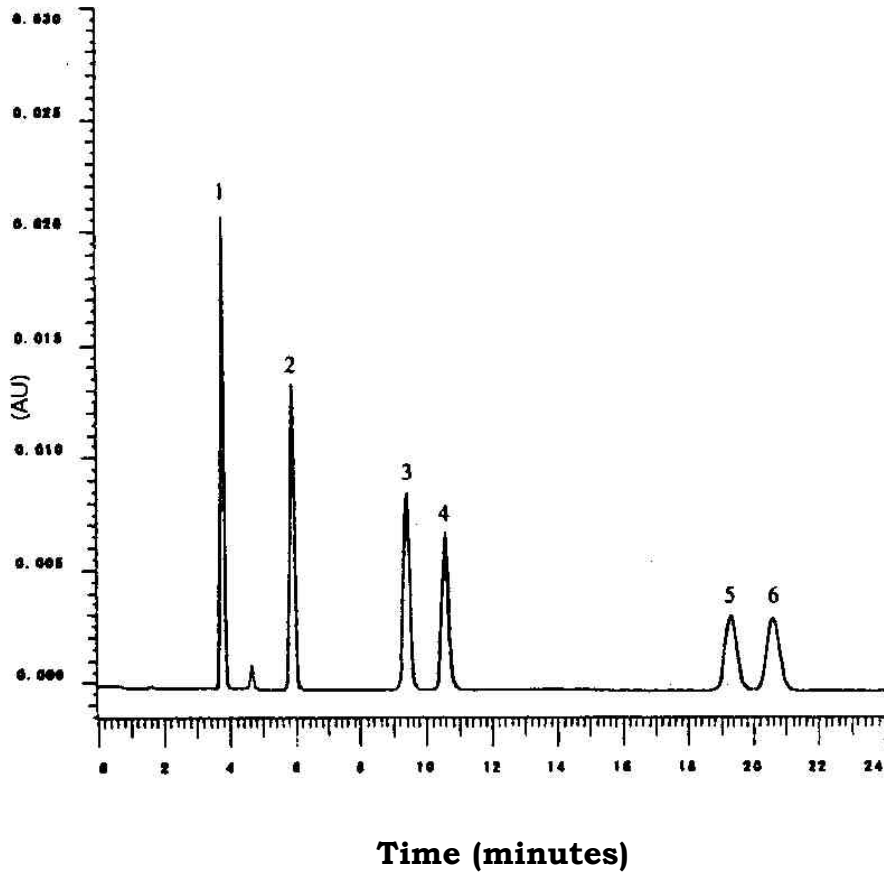

Column	Mightysil RP-18 GP 150-4.6mmØ 5µm
Eluent	Methanol/Water = 1/1
Flow Rate	1.0mL / min.
Detection	UV254nm
Temperature	40°C
Sample Volume	10µL
Samples	1. Methyl p-hydroxybenzoate 1µg/mL 2. Ethyl p-hydroxybenzoate 1µg/mL 3. Isopropyl p-hydroxybenzoate 1µg/mL 4. <i>n</i> -Propyl p-hydroxybenzoate 1µg/mL 5. Isobutyl p-hydroxybenzoate 1µg/mL 6. <i>n</i> -Butyl p-hydroxybenzoate 1µg/mL