


Separation of β -Carotene

Data# F-059

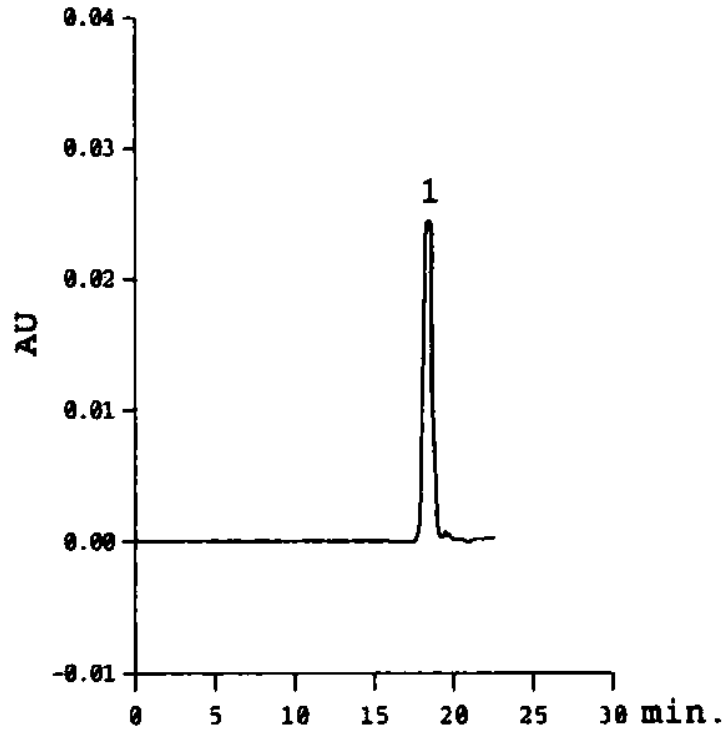

| | |
|----------------|-----------------------------------|
| Column | Mightysil RP-18 GP 250-4.6mmØ 5µm |
| Eluent | Ethanol 100% |
| Flow Rate | 1.0mL / min. |
| Detection | UV-VIS 453nm |
| Temperature | 40°C |
| Sample Volume | 10µl |
| Detected peaks | 1. β -Carotene 2µg/ml |