


Separation of Anthocyanins

Data# F-060

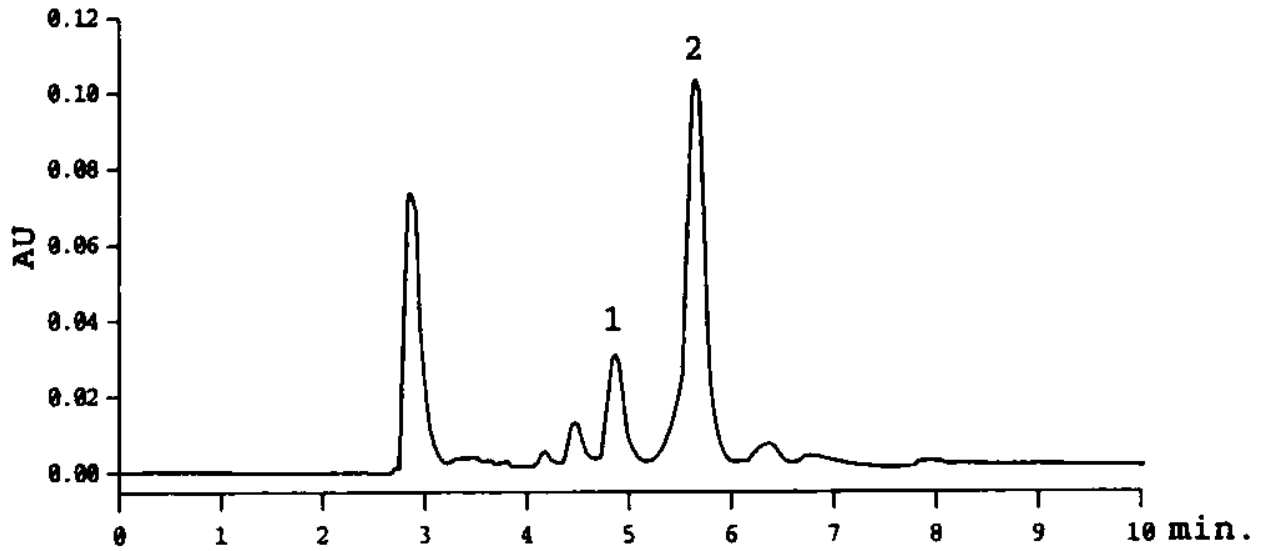

Column	Mightysil RP-18 GP 250-4.6mmØ 5µm	
Eluent	A: 0.5% Trifluoroacetic acid B : Trifluoroacetic acid / Acetonitrile = 50 / 50	
Flow Rate	1.0mL / min.	
Detection	UV-VIS 520nm	
Temperature	40°C	
Sample Volume	10µl	
Detected peaks	1. Acrylanthosyanine	1mg/ml
	2. Anthocyanin	3mg/ml