


## Separation of Allylthiocyanate

Data# F-063

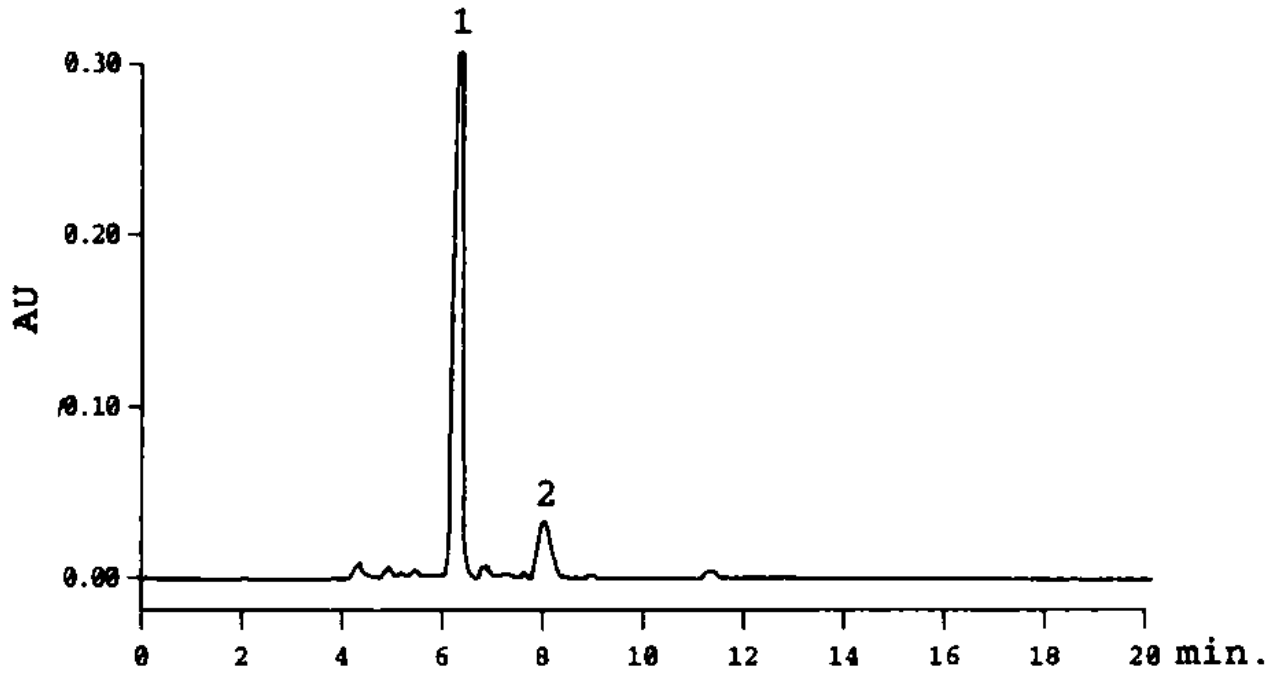

Column	Mightysil RP-8 GP 250-4.6mmØ 5µm	
Eluent	Acetonitrile / Water = 70 / 30	
Flow rate	0.8 ml / min.	
Detection	UV240nm	
Temperature	40°C	
Sample Volume	10µl	
Detected peaks	1. Allyl isothiocyanate	0.4mg/ml
	2. Fenethylcyanate	0.3mg/ml