


Separation of Vitamines

Data# F-067

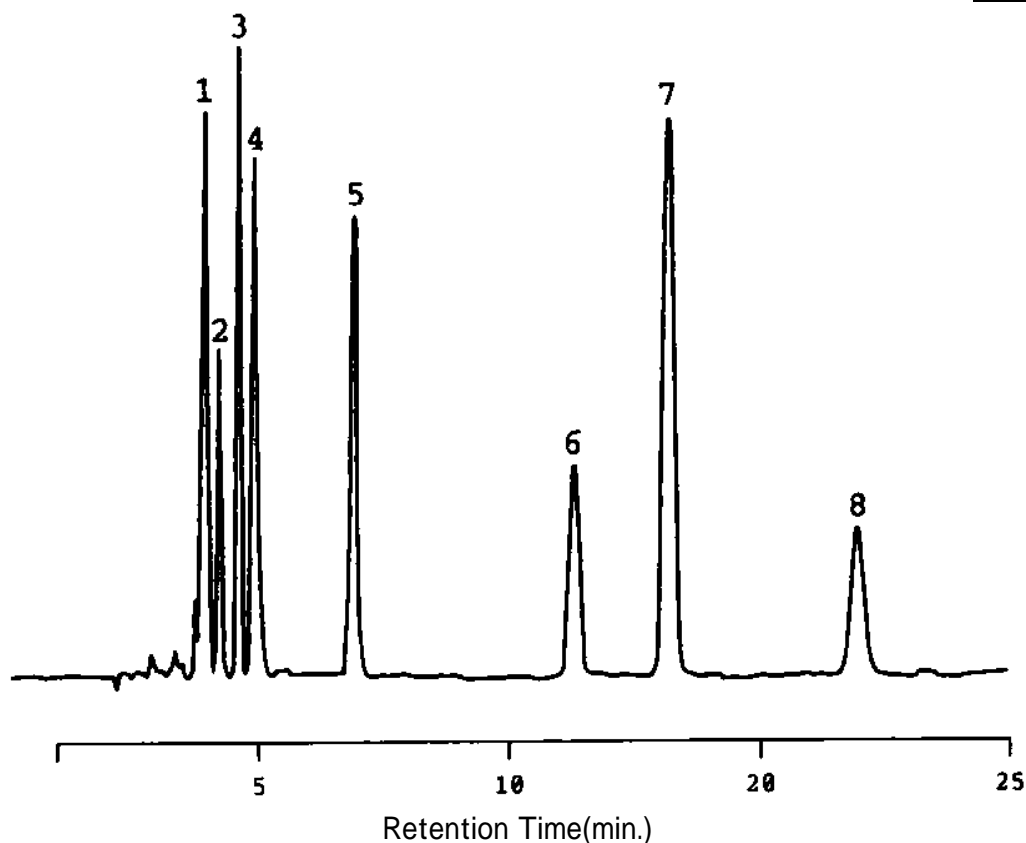

Column	Mightysil RP-18 GP Aqua 250-4.6mmØ 5µm	
Eluent	0.1% Phosphoric acid containing 10mMSodium Hexanesulfonate / Acetonitrile = 90 / 10	
Flow rate	1.0 ml / min.	
Detection	UV210	
Temperature	35°C	
Sample Volume	5µl	
Detected peaks	1. Nicotinic acid	0.05 mg/ml
	2. Pantothenic acid Calcium salt	0.3 mg/ml
	3. Nicotinamide	0.05 mg/ml
	4. Riboflavin phosphate sodium salt	0.2 mg/ml
	5. Pyridoxine hydrochloride	0.05 mg/ml
	6. Riboflavin	0.15 mg/ml
	7. Folic acid	0.05 mg/ml
	8. Thiamine Hydrochloride	0.15 mg/ml