


Separation of Carotenoids

Data# F-071

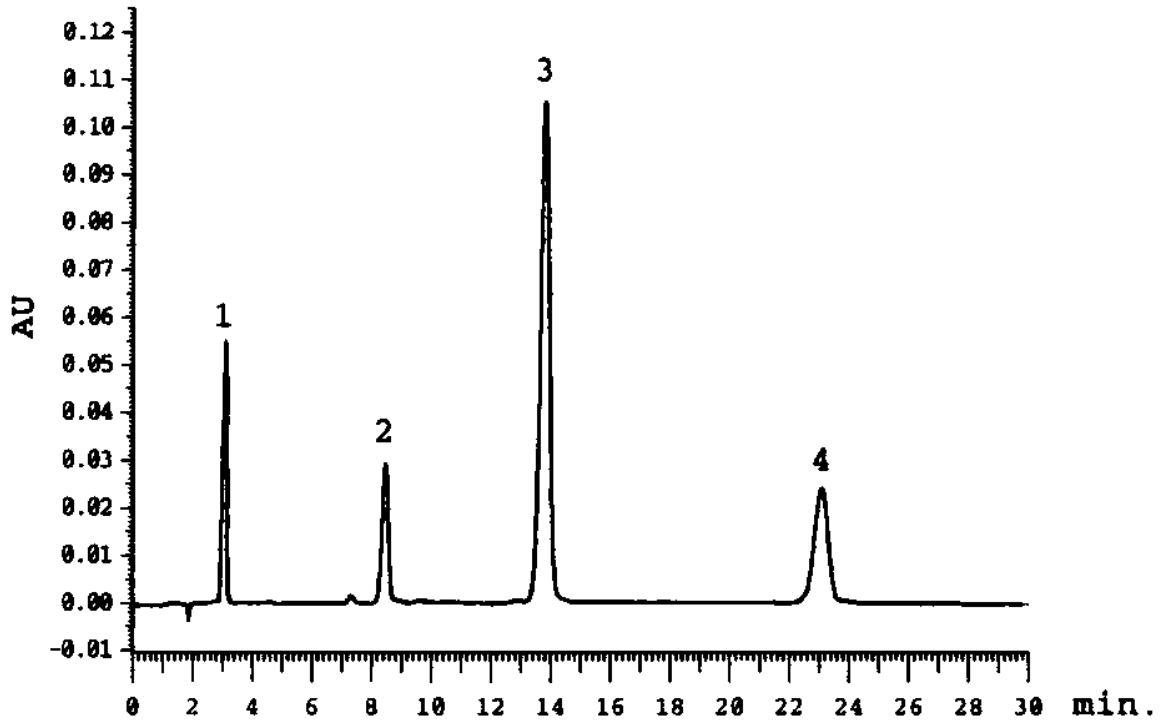

Column	Mightysil RP-18 (L)GP 150-4.6mmØ 5µm	
Eluent	Acetonitrile / Methanol = 50 / 50	
Flow rate	1.0 ml / min.	
Detection	UV460nm	
Temperature	40°C	
Sample Volume	10µl	
Detected peaks	1. Lutein	4 mg/ml
	2. -Cryptoxanthin	2 mg/ml
	3. Lycopene	20 mg/ml
	4. -Cartene	20 mg/ml